

Know Your Oscilloscope

Oscilloscope is an electronic measuring instrument that creates a live and visible two varying in amplitude with respective time.

Vertical corresponds amplitude and horizontal axis corresponds to time.



Oscilloscope can display signals from DC to very high frequencies, up to 200-500MHz.

Oscilloscope can be single channel, 2 channels or 4 channels.

Now a days a number of mathematical calculations such as additions, multiplication, FFT analysis etc. Or possible on CRO.

Fine measurement by using cursor can be done and signals can be stored and transfer and nay other location using digital storage technics.


Block Diagram of Oscilloscope

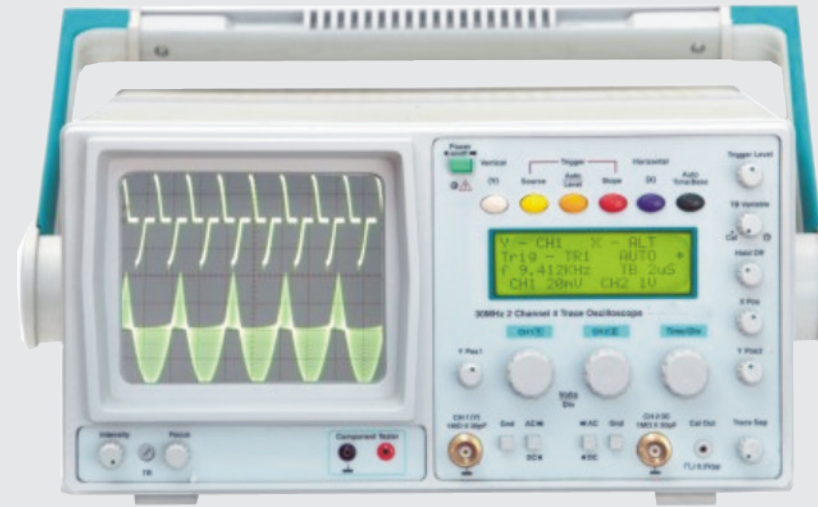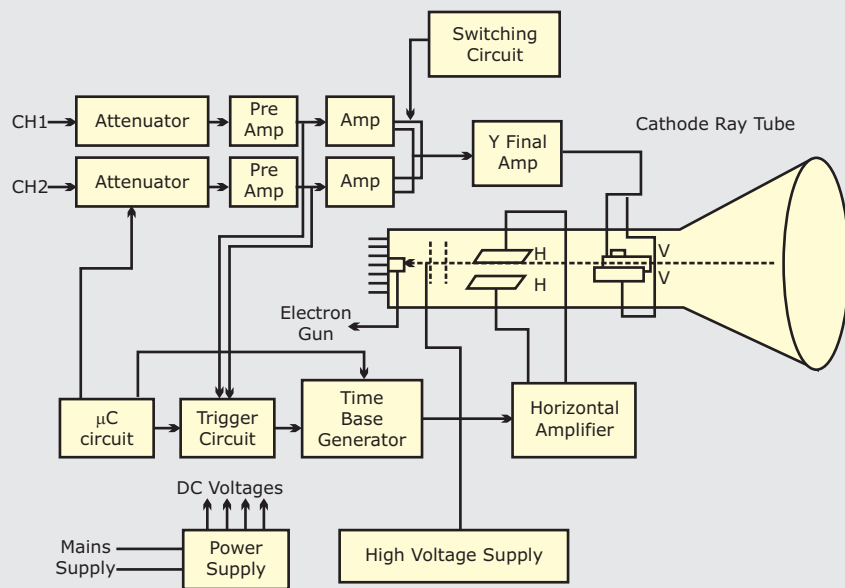

Features:


- ! Auto Time Base
- ! Signal Frequency Display Built in
- ! Large LCD Display
- ! 4- Trace operation (view × 1 & × 10 together)
- ! 30 MHz Bandwidth
- ! × 10 Magnification
- ! 20 ns max Sweep Speed
- ! Stable Triggering up to 50MHz
- ! Alternate Triggering
- ! Variable Hold Off
- ! Component Continuity Tester
- ! Component and Continuity Tester
- ! USB

Function Keys

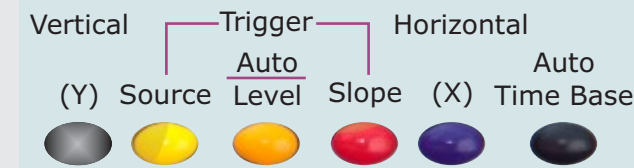


For selecting vertical, Horizontal, trigger and auto time base functions. Vertical key selects various vertical modes of operation such as CH1, CH2, dual etc. Horizontal key selects X1, X10, CT etc. Source key select triggering source like CH1, CH2, external etc. Slope key select +ve or Negative slope for triggering. Auto level key selects auto or level triggering mode. Auto time base key selects automatic working of time base.

Rotary Controls

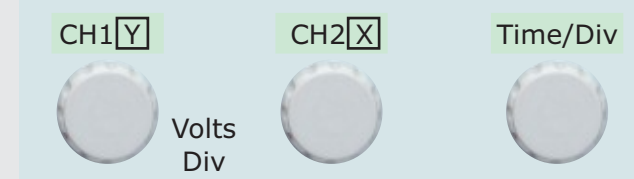

Volts/Div changes the vertical sensitivity of CH1 and CH2 Time/Div changes the time base speeds.

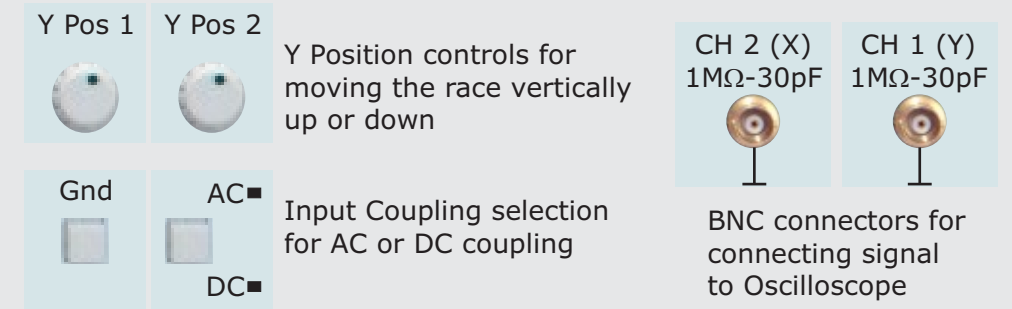


LCD Display




All the parameters adjected by verious key are displayed on LCD


Component Tester

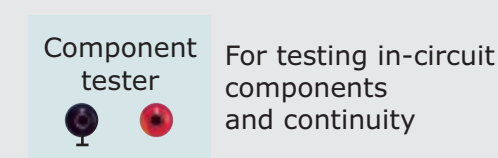


Trigger Controls

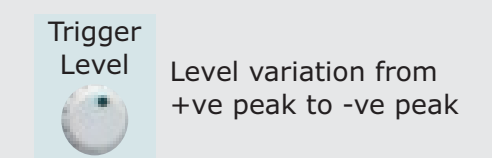

General Controls

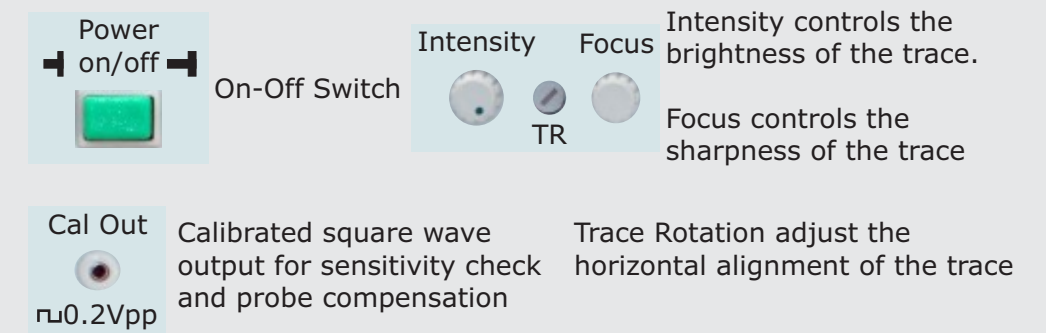

Back Panel Controls

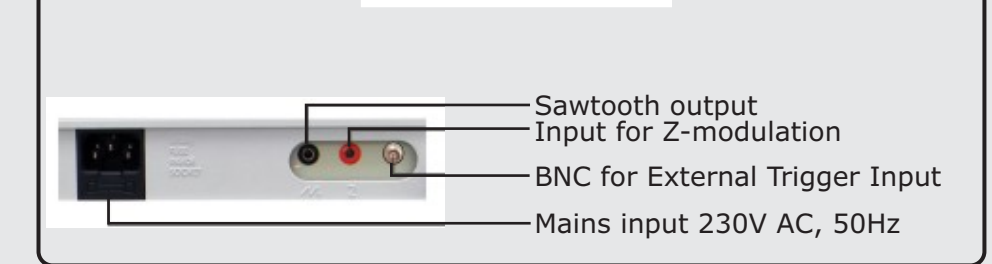

Measurements on Oscilloscope

Vertical Measurement (Input Sinewave)

Volts/Div = 50mV
Deflection Vpp = 4Div
Signal Strength = 50mV × 4 = 200mVpp



Horizontal Measurement (Input Sinewave)

Time = TB speed × Horizontal Distance
Frequency = $\frac{1}{\text{Time in sec}}$ Hz
Time/Div = 1mS
No. Of Div for one cycle = 4 Div
Period of Signal = 4mS
Freq. Of Signal = $\frac{1}{4\text{ms}}$ = 250Hz




DC Measurement (input 5VDC)

Input coupling DC
Volts per div = 2V
Deflection = 2.5 Div
DC voltage 2.5 × 2 = 5V



Rise Time Measurement

Input squarewave

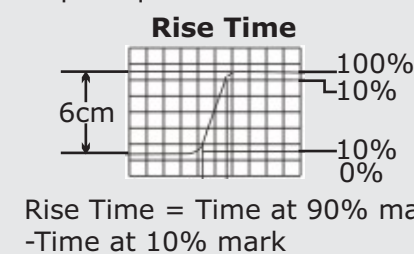

Phase Measurement (X-Y Mode)

Input sinewaves

Phase (X-Y) Mode

